


Medium Back Slings Fitting Protocol



Client Information: Name: Room:

Facility: Lift Used: Hanger Bar Used:

Sling Model: Name/Article Number: Fabric Size

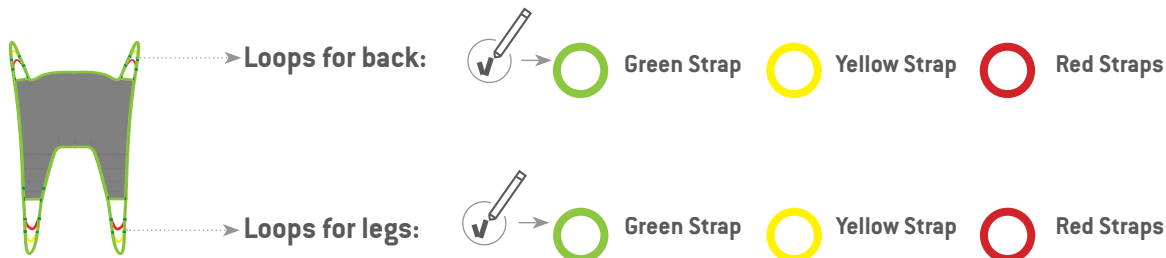


Extension Loops Back:

21180-10 (10cm/3.9")
21180-15 (15cm/5.9")
21180-20 (20cm/7.8")
21180-25 (25cm/9.8")
21180-35 (35cm/13.7")

Extension Loops Legs :


21180-10 (10cm/3.9")
21180-15 (15cm/5.9")
21180-20 (20cm/7.8")
21180-25 (25cm/9.8")
21180-35 (35cm/13.7")

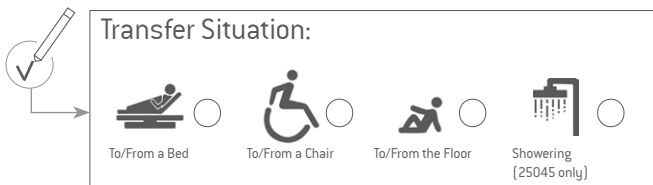


Arm placement:




Leg Placement:

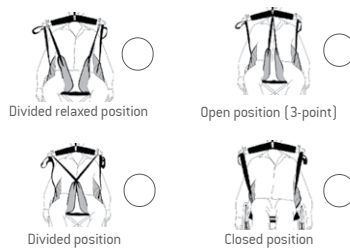

Suspension:

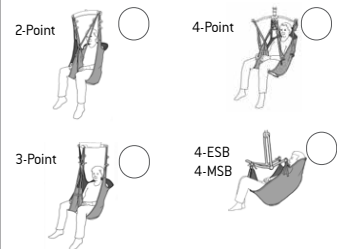

Accessories required:



25102 Reinforced Leg Support - One Size ☐



50866 Upholstered Cover for Hanger Bar ☐
Do not use in wet environments.







Notes:

Fitting Protocol Completed by:

Position/Title:

Date:

Size recommendation:


					
User weight kg/lbs	Client length cm/inch	Client back height* cm/inch	Client hip width* cm/inch	Recommended Size*	Color
15-20 / 33-44	110-130 / 43-51	55-65 / 22-25	23-30 / 9-12	Junior Small (JS)	
20-35 / 44-77	120-150 / 47-59	60-75 / 23-29	29-38 / 11-15	Junior Medium (JM)	
30-60 / 66-132	140-170 / 55-67	70-85 / 27-33	36-42 / 14-17	Small (S)	
55-90 / 121-198	160-190 / 63-75	80-95 / 31-37	41-47 / 16-19	Medium (M)	
85-120 / 187-264	180-206 / 71-81	90-103 / 35-40	46-55 / 18-22	Large (L)	
110-150 / 242-330	180-210 / 81-83	98-107 / 38-44	54-67 / 21-26	Extra Large (XL)	
140-200 / 309-441	180-210 / 81-83	106-110 / 40-46	60-74 / 23-29	Extra Extra Large (XXL)	
190-300 / 419-661	180-210 / 81-83	108-112 / 42-49	63-78 / 25-31	Extra Extra Extra Large (XXXL)	




Visit the **Human Care Slings Size Guide for drawings and measurements of our slings**. You can also find drawings on each sling in the user manual, delivered with the product and available on our websites.

- * To measure the client back height, measure from the clients coccyx to the top of the head.
- * To measure the client hip width (Trochanter), have the client sitting down and measure in a straight line (not the circumference). This gives an indication of the sling's needed aperture width +/- 5cm.

These sizes are recommendations only. A correct fitting must always be carried out by clinically knowledgeable personnel using the sling's user manual. Please be aware that some slings are not available in all sizes. You can find drawings on each sling in the user manual, delivered with the product and available on our websites.

 **SLING TOO LARGE** Patient may slide out.

 **SLING TOO SMALL** Patient is too close to hanger bar/feels too tight on the patient.

Fitting Protocol Completed by:

Name:

Date:

Position/Title:



Important! This fitting protocol does not replace the user manual. Read all instructions before use!